



Public Health
Prevent. Promote. Protect.

**Victoria County Public Health Department
Environmental Health Services Water Lab**

2805 N. Navarro Street Victoria, Texas 77901

Phone (361) 578-6281


Fax (361) 579-6348

Water Sample Bottle Guidelines

All samples must arrive on ice and in the bottles provided by VCPHD Water Laboratory. *Any samples that do not arrive on ice or are frozen will be marked unsuitable and rejected.*

Per TCEQ and Standards Methods 23rd Edition the sample container must have an inch head space. The bottle needs to be filled in the area in-between the 100ml line and the 120 ml line or in-between the 100 ml and the black line in order for the laboratory to stay in compliance.

Samples filled at the 100ml line or over the 120ml/black line will be marked unsuitable and rejected.

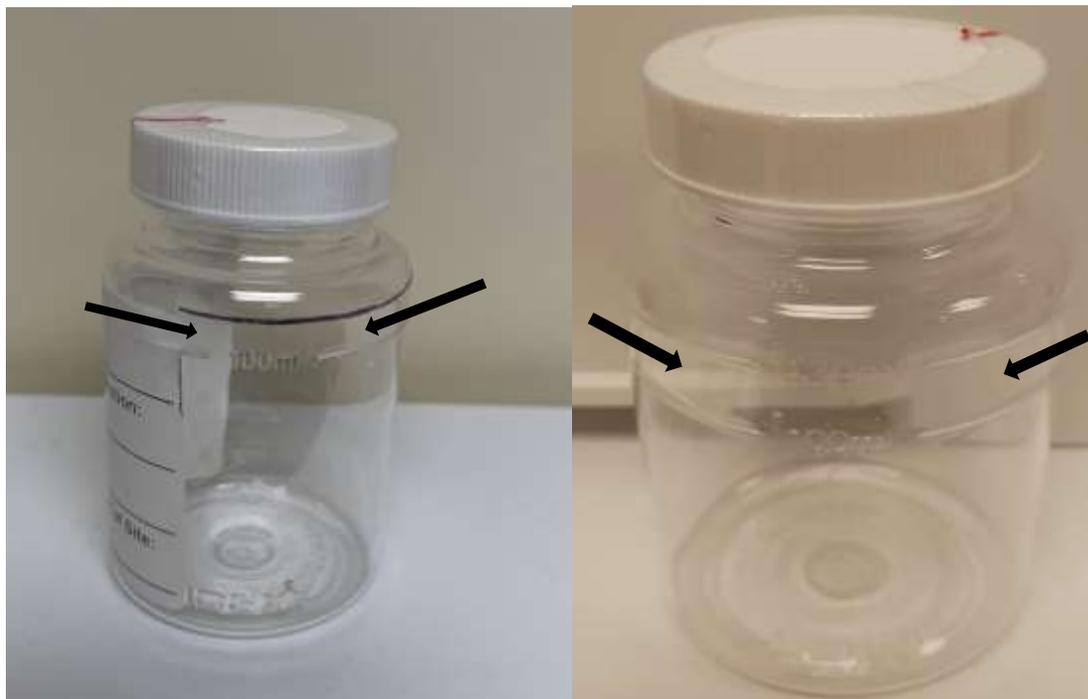

Samples are accepted:

Monday, Tuesday, Wednesday: 8:00am - 11:00am & 1:00pm - 3:00pm

Thursday: 8:00am - 11:00am

*** 2 days before a county holiday * 8:00am - 11:00am**